



INSTRUCTION MANUEL

HOEK TRIAXIAL CELL

Model HTC

© Roctest Limited, 2003. All rights reserved.

This product should be installed and operated only by qualified personnel. Its misuse is potentially dangerous. The Company makes no warranty as to the information furnished in this manual and assumes no liability for damages resulting from the installation or use of this product. The information herein is subject to change without notification.

Tel. : 1.450.465.1113 • 1.877.ROCTEST (Canada, USA) • 33 (1) 64.06.40.80 (Europe) • www.roctest.com • www.telemac.com

TABLE OF CONTENTS

1	INTRODUCTION	1
2	DESCRIPTION	2
3	OPERATING INSTRUCTIONS	4
3.1	ASSEMBLY	4
3.2	TEST PROCEDURES	5
3.3	POST TEST PROCEDURE.....	5
4	MAINTENANCE	6
5	REFERENCES	6

1 INTRODUCTION

The HOEK Triaxial Cell is designed to determine the triaxial strength of diamond drill cores of rock or concrete. Tests carried out on a series of samples under different confining pressure allow the user to determine:

- The strength and elastic properties
- Shear strength at different confining pressures
- Angle of shearing resistance and cohesion
- Modulus of elasticity and Poisson's ratio

One of the most convenient method for determining triaxial strength of rock is to apply a uniform hydraulic pressure to the curved surface of a cylindrical specimen and then to apply a compressive axial load to the rock specimen until failure occurs. Tests are normally done on a series of samples under different confining pressure to study the strength properties of the sample under various stress conditions which simulate natural or arranged levels. Test data may be used to determine the strength and elastic properties of rock, shear strength at various confining pressures, the angle of shearing resistance, cohesion intercept and deformation moduli.

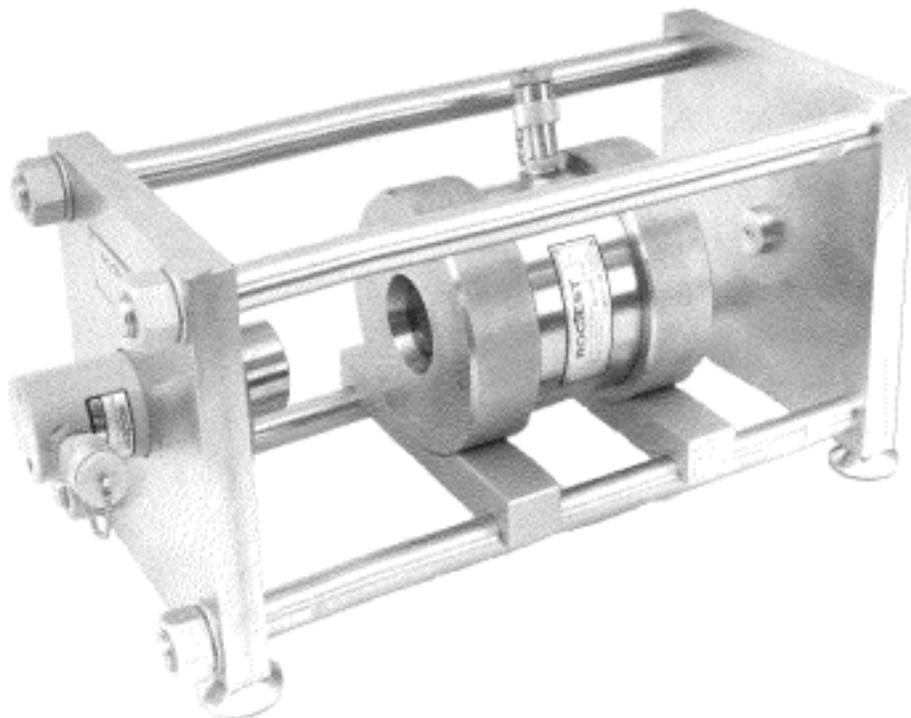


FIGURE 1: HOEK cell in a compression testing frame

2 DESCRIPTION

The HOEK cell consists of a hollow steel cylinder with threaded removable end caps. A urethane rubber membrane with U-shaped end seals, form a pressurization chamber for hydraulic fluid. The rubber membrane has a tensile strength of over 38 MN/m² and a durometer of 95, compared with values of about 21 MN/m² strength and a hardness varying from 30 to 90 in the case of natural rubber. The cell comprises an inlet fitted with a 3/8" NPT male quick-connect and an air outlet plug to saturate the pressurization chamber.

The cell is supplied with a pair of spherical seats (optional) to apply the axial load to the flattened ends of the sample. These seats are made of tool steel hardened and ground to ASTM (D2664) standard. An additional design feature is the clearance gap between the cell body and the end platens, which allows the passage of the strain gauge wiring out of the cell without having to pass it through the rubber membrane and hydraulic fluid.

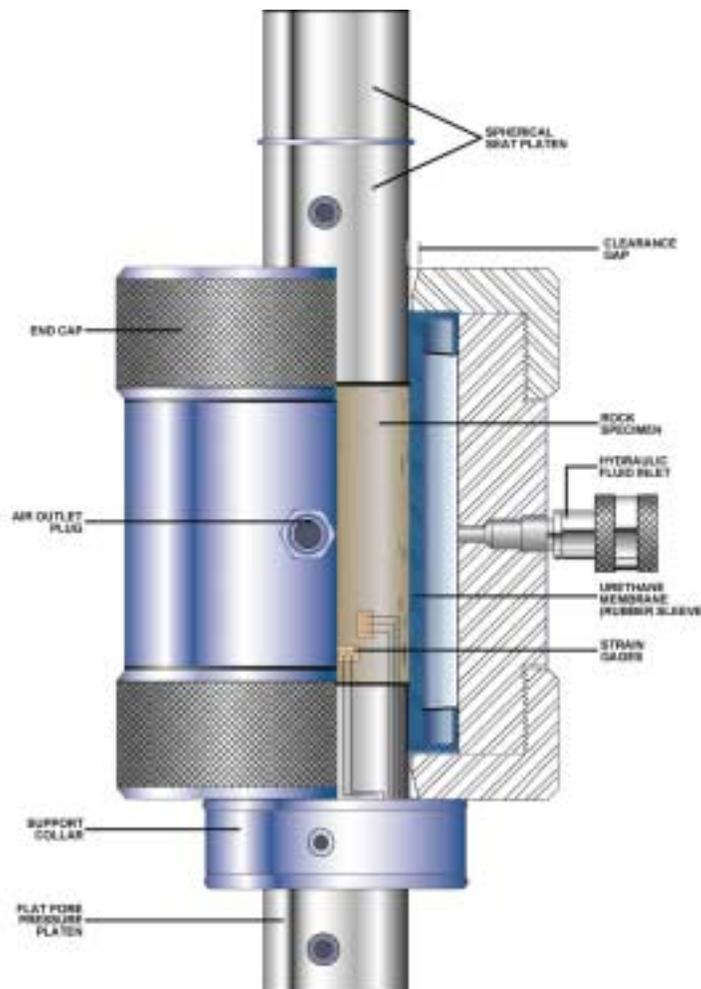


FIGURE 2: Schematic view of HOEK triaxial cell

As illustrated on **Figure 3**, hydraulic fluid is retained within the annular space created between the rubber membrane and the cylinder. The membrane has integrated "U" seals at each end and a threaded steel cylinder. This configuration makes it possible to test and remove the rock specimen without having to replace the seals.

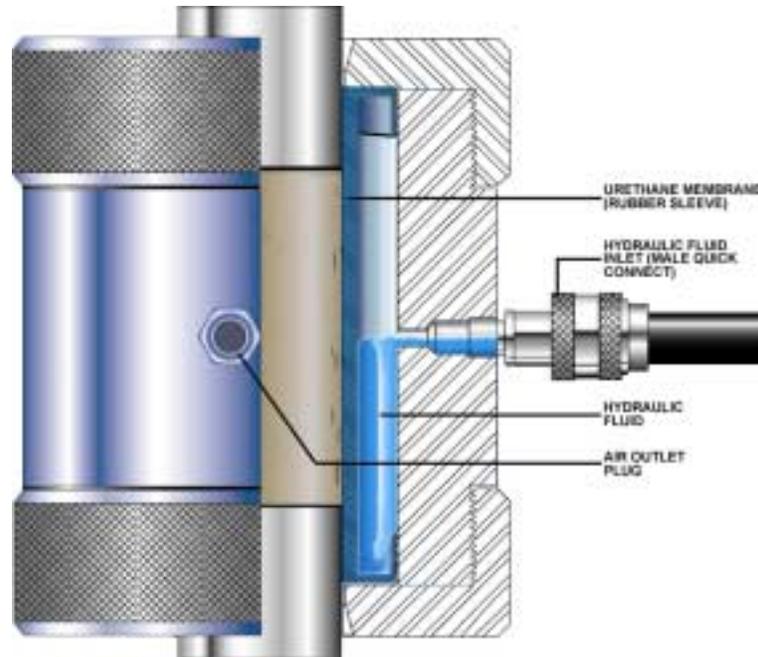


FIGURE 3: HOEK cell

The spherical seat platens are manufactured from high quality steel and are used without lubrication so that, once under a load, they are effectively locked together and react as one. In this manner, they compensate for any initial misalignment of the specimen ends.

To achieve consistent and reliable test results, it is recommended that cylindrical samples having a length to diameter ratio of at least 2 are tested (in references 1, 2 and 3) and the ends be ground flat to within 0.025 - 0.012 mm dependant of sample diameter. Reference 4 concisely describes the tolerance of specimen preparation for sample laboratory testing in uniaxial compression and is equally applicable to this situation.

3 OPERATING INSTRUCTIONS

3.1 ASSEMBLY

1. Remove end caps from cell, inspect cell and make sure that all internal surfaces on both cell and end caps are clean and free from surface irregularities.
2. Make sure the rubber membrane is clear from all blemishes.
3. Coat the inside of body cell with hydraulic oil to give rubber membrane an easy fit. The rubber is slightly oversized and must be installed carefully inside the cell.
4. After rubber membrane installation, put end caps back on cell (when all mating surfaces are clean and free of grit). Hand tightness is all that is required.

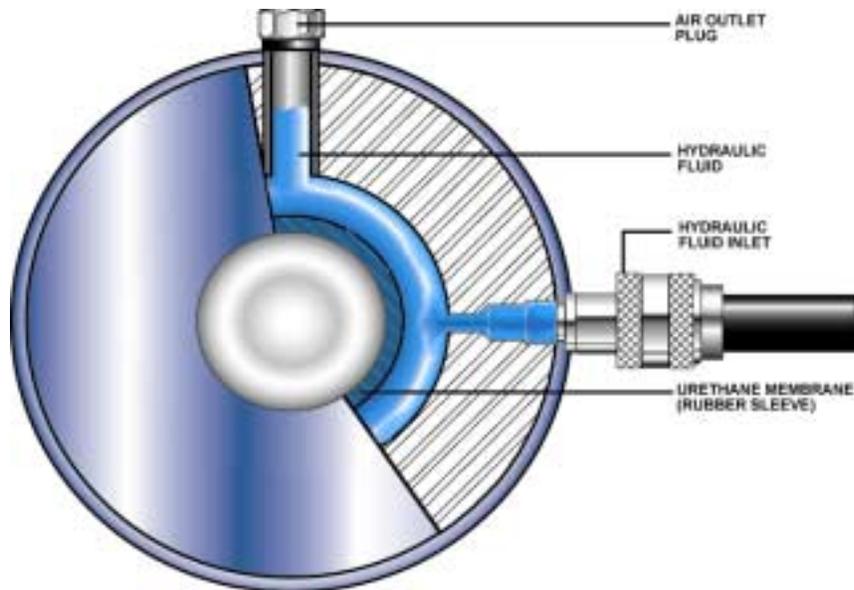


FIGURE 4: Filling HOEK cell with hydraulic fluid

5. Hold cell with the air outlet upwards, unscrew the plug lightly, and using hand pump, saturate the cell with hydraulic fluid. The cell should be completely air free. Tighten back the plug.
6. The cell is now ready to be used.

3.2 TEST PROCEDURES

1. The ends of the rock specimen (a minimum length to a diameter ratio of 2) must be ground flat within a parallelism of 0.025 mm to 0.012 mm depending on the diameter of the sample.

NOTE: MAKE SURE ROCK SPECIMEN IS WELL CENTERED INTO THE CELL'S RUBBER MEMBRANE.

2. After saturation of the pressurization chamber, the cylindrical rock sample is inserted into the chamber within the confining membrane. The two spherical seats are positioned so that the rock core lies centrally in the triaxial chamber.
3. After applying a small confining pressure to hold the rock core in place, the cell with its spherical seats is placed in the loading frame and a small axial load is applied to hold the system firmly in place.
4. To determine Poisson's ratio, 2 orthogonal strain gages are glued on the rock core. The strain gages are read during the test with a Wheatstone bridge readout. The triaxial test may then be run after adjustment of the confining pressure to the required value.
5. With the use of strain gages, triaxial tests run on the same type of rocks at different confining pressures allow the determination of the failure envelope with the angle of friction and cohesion, the modulus of elasticity and Poisson's ratio.
6. Axial load of rock sample may begin.

3.3 POST TEST PROCEDURE

1. Once rupture is reached and completed, release confining pressure and axial load while making sure the cell does not fall from the load frame.
2. Remove the cell and spherical seats from the load frame, then remove spherical seats from the cell.
3. Unless the specimen is severely deformed, it may be removed from the cell with little force without dismantling the cell. However, if the sample is severely deformed, then the cell should be dismantled, and the sample debris removed. The use of excessive forces to remove fractured rock sample is not recommended, and may damage the rubber membrane.

4 MAINTENANCE

It is important to maintain the HOEK cell clean and to regularly inspect all components especially all platen and seat surfaces, non-observance will lead to premature failure of the membranes, and general reduction of mating tolerance resulting in hydraulic fluid leaks and sample contamination.

Furthermore, rock debris left on spherical seatings or on the cylinder ends may lead to stress concentration during loading, producing premature sample failure and platen deterioration.

5 REFERENCES

- 1) **Hoek E. & Franklin J.A. Simple.** Triaxial Cell for Field or Laboratory Testing of Rock. Trans. Inst. Min. Metall. (Sect. A: Min. Industry), 1968, A22-26.
- 2) **Jaeger J.C. & Cook N.G.** Fundamentals of Rock Mechanics. (London: Methuen, 1969, USA distributors: Barnes & Noble Inc.).
- 3) **Jaeger J.C.** Brittle Fracture of Rocks. In Failure and Breakage of Rock. (Fairhurst C. ed. (New York: AIME 1067), 3-57.
- 4) **Hawkes I. & Mellor M.** Uniaxial Testing in Rock Mechanics Laboratories. Eng. Geol., 4, (1970), 177-285.